smiths medical
bringing technology to life



CADD®-Solis VIP Ambulatory Infusion System

Alarm Help Screens

When certain alarms occur, additional information may be displayed on the screen.
The help screens describe what you can do to try to solve the problem that is causing the alarm.


Steps:

1. When an alarm occurs, press **SILENCE** to quiet the alarm.
2. If help screens are available for the alarm, "Help" appears above the right soft key. To view the help screens, select **HELP**.
3. Follow the applicable instructions provided on the help screen. To page through all of the available help screens, press **NEXT** repeatedly. Press **ACKNOWLEDGE** at any time to exit Help.
4. "Retry Help" appears when no additional help steps are available. To page through the help screens again, press **RETRY HELP**. The alarm screen reappears as in Step 2 above. Repeat steps 2 and 3. When the alarm clears, the help screen will no longer be displayed.

The following alarms have associated help screens. Refer to steps above to navigate the help screens.

Cannot start pump without a latched cassette.




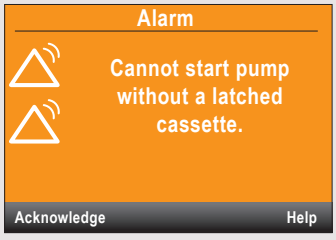








Upstream occlusion. Clear occlusion between pump and reservoir.

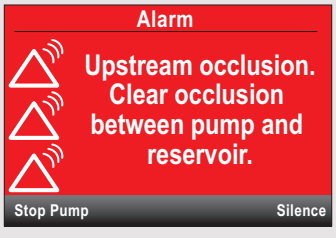


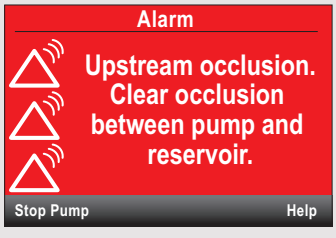

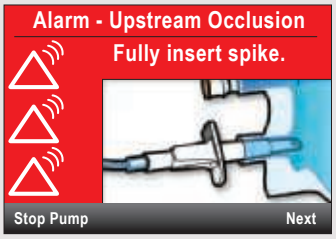

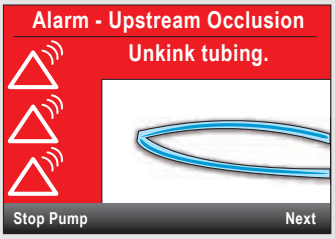




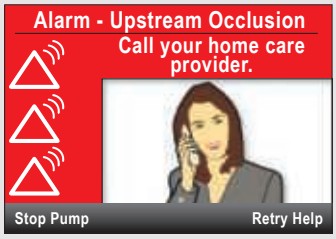



CADD®-Solis VIP Ambulatory Infusion System
Alarm Help Screens


The following alarms have associated help screens. Refer to steps to navigate the help screens.


Downstream occlusion. Clear occlusion between pump and patient.

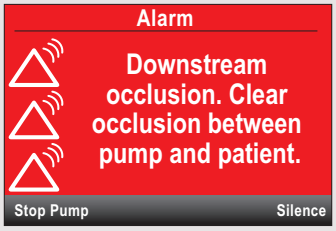


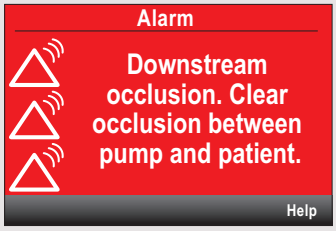


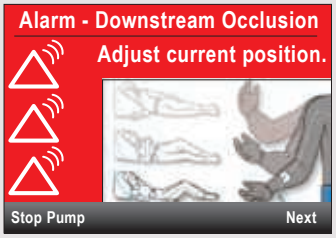

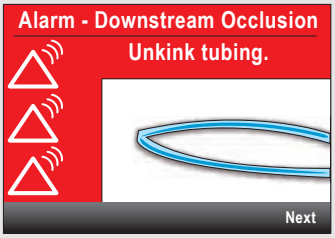

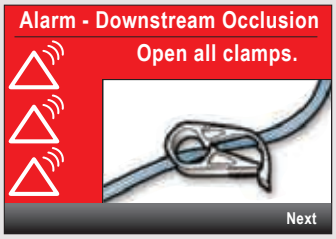

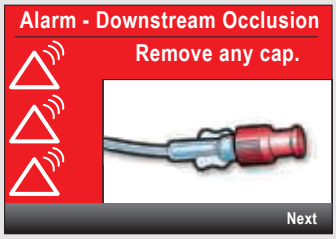

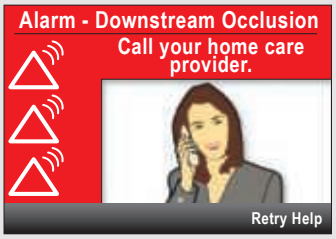

Cannot start pump without a latched and locked cassette. (PCA only)










Lock cassette to start pump. (PCA only)







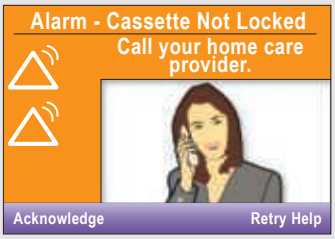

PRODUCT(S) DESCRIBED MAY NOT BE LICENSED OR AVAILABLE FOR SALE IN CANADA AND OTHER COUNTRIES

Smiths Medical ASD, Inc.
St. Paul, MN 55112, USA
Phone: 1-614-210-7300
Toll-Free USA 1-800-258-5361
www.smiths-medical.com

Find your local contact information at: www.smiths-medical.com/customer-support

MPAUCA-1285

Rx ONLY

smiths medical

Smiths Medical is part of the global technology business Smiths Group plc. Please see the Instructions for Use/Operator's Manual for a complete listing of the indications, contraindications, warnings and precautions. CADD and the Smiths Medical design mark are trademarks of Smith Medical. The symbol ® indicates the trademark is registered in the U.S. Patent and Trademark Office and certain other countries. All other names and marks mentioned are the trademarks or service marks of their respective owners. ©2015 Smiths Medical. All rights reserved. IN193583EN-102015